



---

Uludag University Engineering Faculty  
Textile Engineering Lab  
16059 Bursa, Turkey  
Tel : +90 (224) 294 20 64  
Fax : +90 (224) 294 19 03

---



March 18, 2015

**Attention to Lüksteks Oto Döşeme Malzemeler Ted Şirketi,**


The antibacterial activities of samples which you sent us are qualitatively evaluated according to test method AATCC 147 in Laboratory of Medical Microbiology, Medical School in Uludag University and the antibacterial results against both the Gram-positive (*Staphylococcus aureus* - ATCC 6538) and the Gram-negative (*Escherichia coli* - ATCC 35218) bacteria are given in the appendix.

Best Regards.




  
Assoc.Prof. Mehmet Orhan

**Appendix 1. Final Report (Two pages)**

Appendix 1. Final Report (Two pages)

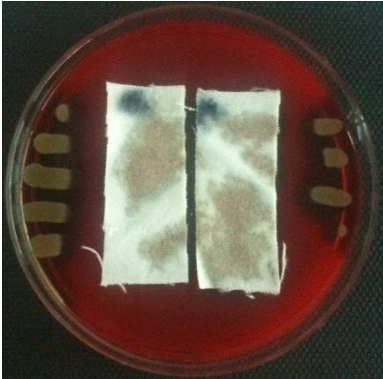

Control fabric

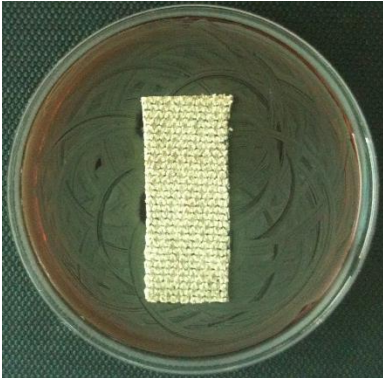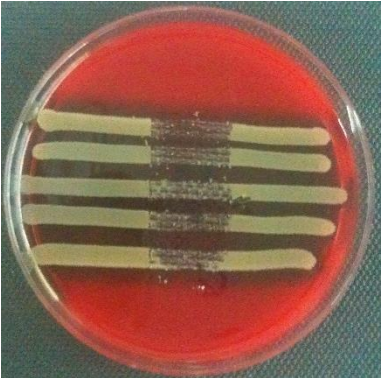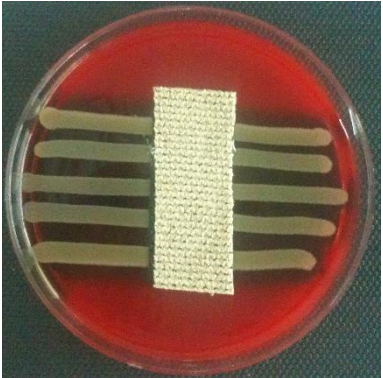



Sample fabric



Figure 1. The antibacterial activities against *Staphylococcus aureus* (ATCC 6538) according to test method AATCC 147



**Control fabric**

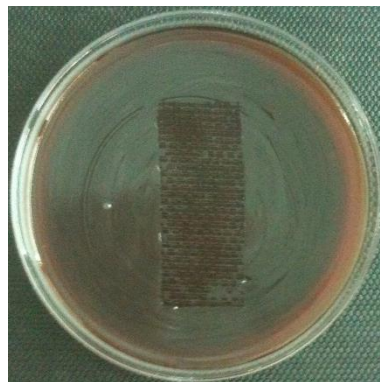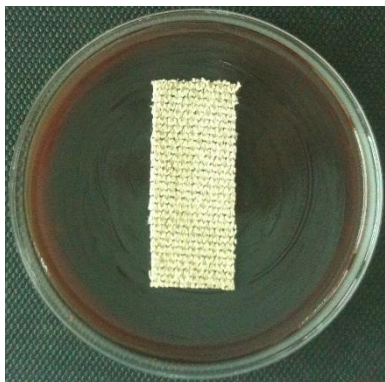

**Sample fabric**

**Figure 2.** The antibacterial activities against *Escherichia coli* (ATCC 35218) according to test method AATCC 147

**Conclusion:** To constitute acceptable antibacterial activity, there must be no bacterial colonies directly under the sample in the contact area. Therefore, the samples has been found to have good antibacterial effect against both the Gram-positive (*Staphylococcus aureus* - ATCC 6538) and the Gram-negative (*Escherichia coli* - ATCC 35218) bacteria.